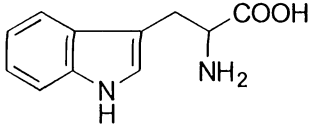
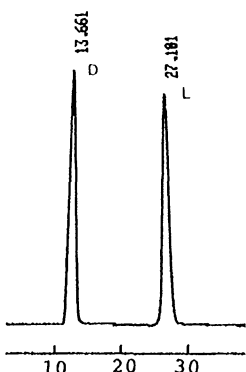

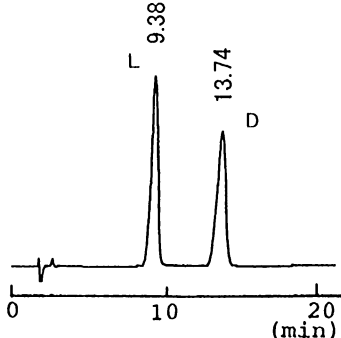

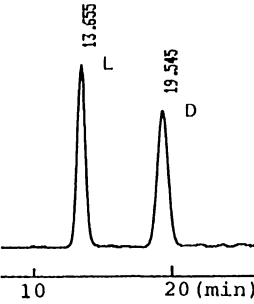

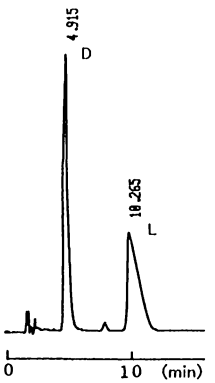

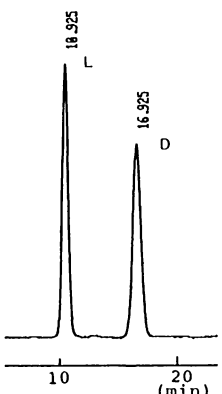
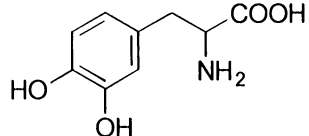
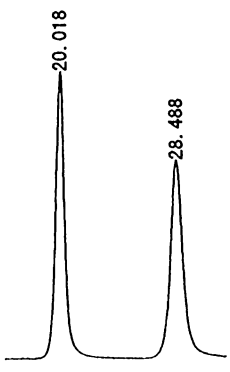
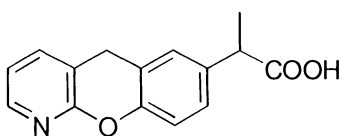
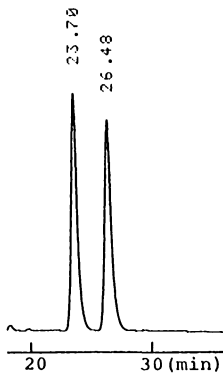
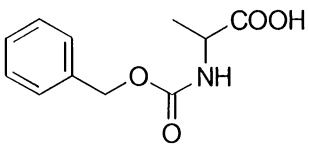
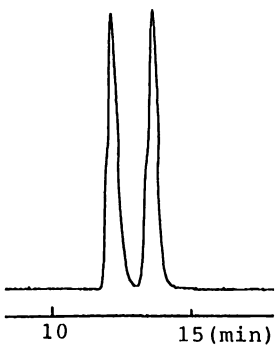


**Group A**

A-01~A-08

<p><b>A-01</b>     <b>Tryptophan</b></p>  <p>OA-6100 Column:4.6mmI.D.×15cm Mobile phase:2mmol/L copper (II) sulfate in water/acetonitrile (90:10) Flow rate:1.0mL/min    Detector:UV254nm Injection:3µL (4mg/mL)</p> 	<p><b>A-02</b>     <b>Phenylalanine</b></p>  <p>OA-5000 Column:4.6mmI.D.×15cm Mobile phase:2mmol/L copper (II) sulfate in water/2-propanol (85:15) Flow rate:1.0mL/min Detector:UV254nm</p> 		
<p>OA-6100    2.10 { D, L } OA-5500    2.05 { D, L } OA-8000    1.29 { D, L }</p>	<p>OA-4800    1.21 { L, D } OA-5000    1.11 { L, D }</p>	<p>OA-6100    4.07 { D, L } OA-6000    2.70 OA-5500    1.74 { D, L }</p>	<p>OA-5000    1.55 { L, D } OA-4800    1.34 { L, D } OA-8000    1.25</p>
<p><b>A-03</b>     <b>Tyrosine</b></p>  <p>OA-5000 Column:4.6mmI.D.×15cm Mobile phase:2mmol/L copper (II) sulfate in water/2-propanol (95:5) Flow rate:1.0mL/min    Detector:UV254nm Injection:3µL (3mg/mL)</p> 	<p><b>A-04</b>     <b>Histidine</b></p>  <p>OA-6100 Column:4.6mmI.D.×15cm Mobile phase:2mmol/L copper (II) sulfate in water/acetonitrile (95:5) Flow rate:1.0mL/min Detector:UV254nm    Injection:3µL (6mg/mL)</p> 		
<p>OA-6100    2.21 { D, L } OA-5500    2.08 { D, L } OA-6000    1.79 { D, L }</p>	<p>OA-5000    1.48 { L, D } OA-8000    1.44</p>	<p>OA-6100    2.52 { D, L } OA-6000    2.06 { D, L } OA-5000    1.37 { D, L }</p>	<p>OA-5500    1.18 { D, L } OA-8000    1.14</p>
<p><b>A-05</b>     <b>Phenylglycine</b></p>  <p>OA-5000 Column:4.6mmI.D.×15cm Mobile phase:2mmol/L copper (II) sulfate in water/2-propanol (95:5) Flow rate:1.0mL/min    Detector:UV254nm Injection:5µL (1.5mg/mL)</p> 	<p><b>A-06</b>     <b>DOPA</b></p>  <p>OA-8000 Column:4.6mmI.D.×25cm Mobile phase:hexane/ethanol/trifluoroacetic acid/water (70:30:0.5:0.5) Flow rate:0.7mL/min    Detector:UV254nm Injection:2µL (5mg/mL)</p> 		
<p>OA-6100    3.46 { D, L } OA-6000    1.89 { D, L } OA-5000    1.63 { L, D }</p>	<p>OA-5500    1.24 { D, L } OA-4800    1.16</p>	<p>OA-6100    1.99 { D, L } OA-8000    1.54 OA-5000    1.27 { L, D }</p>	<p>OA-4800    1.14 { L, D } OA-4900    1.09</p>
<p><b>A-07</b>     <b>Pranoprofen</b></p>  <p>OA-2500 Column:4.6mmI.D.×25cm Mobile phase:0.02mol/L ammonium acetate in methanol Flow rate:0.8mL/min Detector:UV254nm</p> 	<p><b>A-08</b>     <b>Z-alanine</b></p>  <p>OA-3200 Column:4.0mmI.D.×25cm Mobile phase:0.01mol/L ammonium acetate in methanol Flow rate:1.0mL/min Detector:UV254nm</p> 		
<p>OA-2500    1.13 OA-3200    1.07 AGP        1.15</p>		<p>OA-3200    1.16 OA-4400    1.08 { L, D } OA-3300    1.05</p>	