
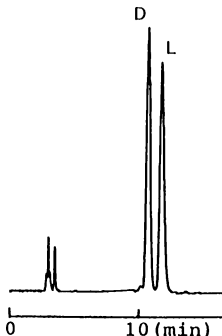

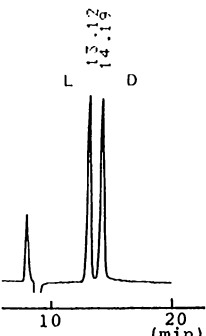

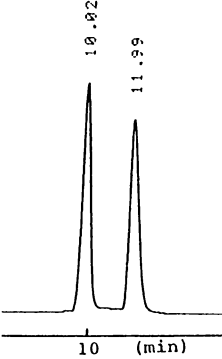

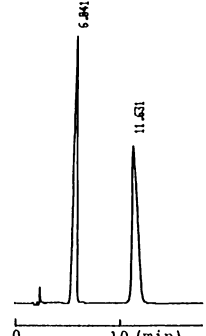

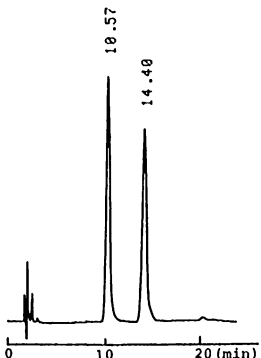

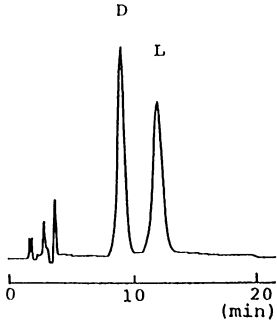

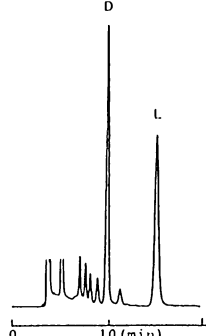

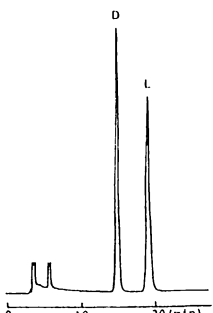


<p>A-22 N-Benzoylglutamic acid</p>  <p>OA-3300 Column:4.0mmI.D.×25cm Mobile phase:0.01mol/L ammonium acetate in methanol Flow rate:1.0mL/min Detector:UV254nm</p> 		<p>A-23 BOC-phenylalanine</p>  <p>OA-4700 Column:4.6mmI.D.×25cm Mobile phase:hexane/2-propanol/methanol/trifluoroacetic acid(98:1:1:0.2) Flow rate:1.0mL/min Detector:UV254nm Injection:2µL (16mg/mL)</p> 	
<p>OA-3300 1.14 OA-3200 1.09</p>		<p>OA-4700 1.11 { L, D } OA-4400 1.10 { L, D } OA-3300 1.09</p>	<p>OA-4000 1.06</p>
<p>A-24 Baclofen</p>  <p>OA-5000 Column:4.6mmI.D.×15cm Mobile phase:2mmol/L copper (II) sulfate in water/2-propanol (85:15) Flow rate:1.0mL/min Detector:UV254nm</p> 		<p>A-25 threo-3-Phenylserine</p>  <p>OA-6100 Column:4.6mmI.D.×15cm Mobile phase:2mmol/L copper (II) sulfate in water/acetonitrile (95:5) Flow rate:1.0mL/min Detector:UV254nm Injection:5µL (5mg/mL)</p> 	
<p>OA-6000 1.69 OA-5000 1.23 OA-4800 1.20</p>		<p>OA-6100 2.20 OA-6000 1.62 OA-4800 1.18</p>	<p>OA-5000 1.15 OA-4900 1.08</p>
<p>A-26 Naphthylglycine</p>  <p>OA-5000 Column:4.6mmI.D.×15cm, 60°C Mobile phase:2mmol/L copper (II) sulfate in water/2-propanol (85:15) Flow rate:1.0mL/min Detector:UV254nm</p> 		<p>A-27 p-Boronophenylalanine</p>  <p>OA-5000 Column:4.6mmI.D.×15cm Mobile phase:2mmol/L copper (II) sulfate in water/2-propanol (90:10) Flow rate:1.0mL/min Detector:UV254nm</p> 	
<p>OA-6100 1.91 { D, L } OA-5000 1.42</p>		<p>OA-5000 1.36</p>	
<p>A-28 O-(3,5-Dinitrophenyl) amino-carboxyllactic acid</p>  <p>OA-3100 Column:4.6mmI.D.×25cm Mobile phase:0.03mol/L ammonium acetate in methanol Flow rate:1.0mL/min Detector:UV254nm</p> 		<p>A-29 O-(3,5-Dinitrophenyl) amino-carboxylmandelic acid</p>  <p>OA-3200 Column:4.6mmI.D.×25cm Mobile phase:0.03mol/L ammonium acetate in methanol Flow rate:1.0mL/min Detector:UV254nm</p> 	
<p>OA-3100 1.79 { D, L } OA-3200 1.77 { D, L } OA-3300 1.31 { L, D }</p>		<p>OA-3100 1.36 { D, L } OA-3200 1.35 { D, L }</p>	