
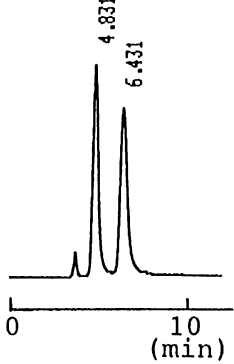

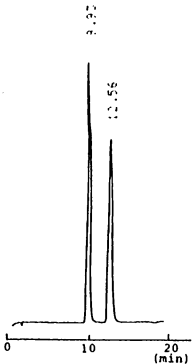

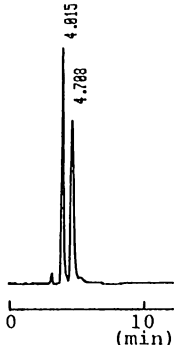

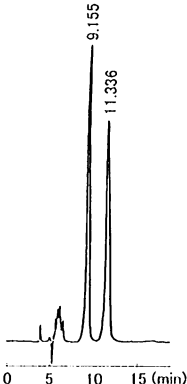

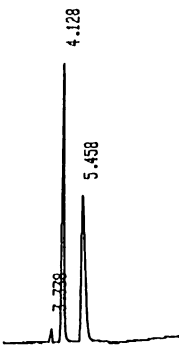

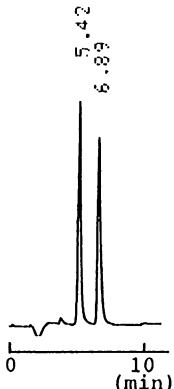

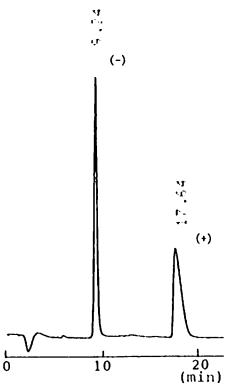
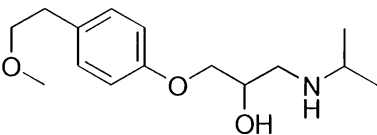
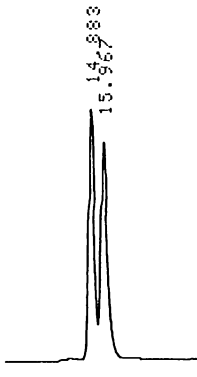


<p><b>B-16</b>     <u>Octopamine</u></p>  <p>OA-6000 Column:4.6mmI.D.×15cm Mobile phase: 0.5mmol/L copper (II) sulfate in water Flow rate:1.0mL/min Detector:UV254nm</p> 	<p><b>B-17</b>     <u>Norphenylephrine</u></p>  <p>OA-5000 Column:4.6mmI.D.×15cm Mobile phase:0.2mmol/L copper (II) acetate and 0.1mol/L ammonium acetate in water (pH 6.5) Flow rate:1.0mL/min     Detector:UV280nm</p> 		
<p>OA-6000    1.47 OA-5500    1.30 OA-5000    1.15</p>	<p>CBH        2.56</p>	<p>OA-5000    1.31 OA-5500    1.23 OA-6000    1.20</p>	
<p><b>B-18</b>     <u>Normetanephrine</u></p>  <p>OA-6000 Column:4.6mmI.D.×15cm Mobile phase: 0.5mmol/L copper (II) sulfate in water Flow rate:1.0mL/min Detector:UV254nm</p> 	<p><b>B-19</b>     <u>Norephedrine</u></p>  <p>OA-8000 Column:4.6mmI.D.×25cm Mobile phase:hexane/ethanol/trifluoroacetic acid (70:30:0.5) Flow rate:0.7mL/min     Detector:UV254nm Injection:2µL (20mg/mL)</p> 		
<p>OA-6000    1.28 OA-5000    1.15 OA-5500    1.15</p>	<p>CBH        2.05</p>	<p>OA-8000    1.44</p>	
<p><b>B-20</b>     <u>p-Hydroxynorephedrine</u></p>  <p>OA-6000 Column:4.6mmI.D.×15cm Mobile phase: 0.5mmol/L copper (II) sulfate in water Flow rate:1.0mL/min Detector:UV254nm</p> 	<p><b>B-21</b>     <u>Phenylglycinol</u></p>  <p>OA-5500 Column:4.6mmI.D.×15cm Mobile phase: 1mmol/L copper (II) sulfate in water Flow rate:1.0mL/min Detector:UV254nm</p> 		
<p>OA-6000    1.53 OA-8000    1.50 OA-5000    1.43</p>	<p>OA-5500    1.13 OA-4900    1.12</p>	<p>OA-5500    1.35 OA-8000    1.08</p>	
<p><b>B-22</b>     <u>Phenylalaninol</u></p>  <p>OA-5500 Column:4.6mmI.D.×15cm Mobile phase: 1mmol/L copper (II) sulfate in water Flow rate:1.0mL/min Detector:UV254nm</p> 	<p><b>B-23</b>     <u>Metoprolol</u></p>  <p>OA-4900 Column:4.0mmI.D.×25cm Mobile phase:hexane/1,2-dichloroethane/ethanol/trifluoroacetic acid (240:140:20:1) Flow rate:1.0mL/min Detector:UV254nm</p> 		
<p>OA-5500    2.04 { -, + }</p>		<p>OA-4900    1.09 AGP        1.26 CBH        1.26</p>	