
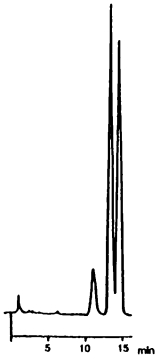

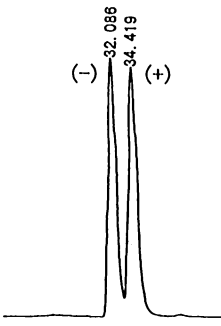

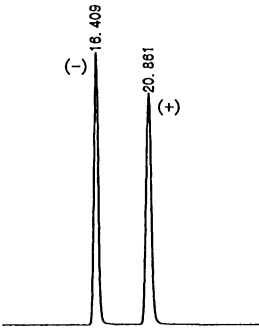

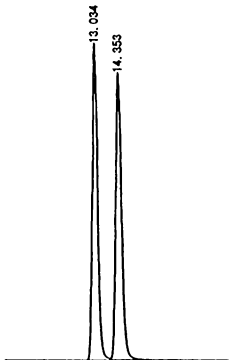

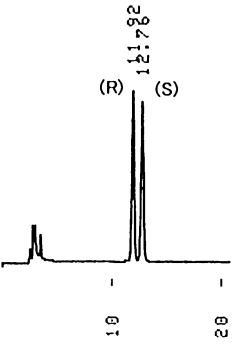

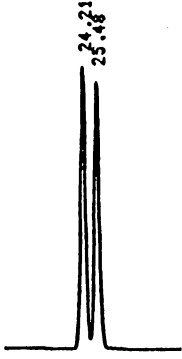

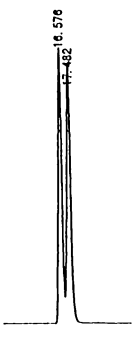

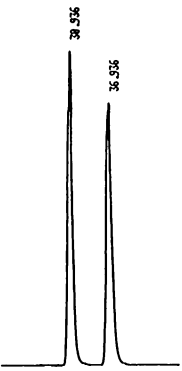


<p><b>E-01</b>     <b>1-Phenylethylalcohol</b></p>  <p>OA-7500 Column:4.6mmI.D.×25cm Mobile phase: water/methanol (75:25) Flow rate:0.7mL/min Detector:UV260nm</p> 	<p><b>E-02</b>     <b>1-(1-Naphthyl)-ethylalcohol</b></p>  <p>OA-2500I Column:4.6mmI.D.×25cm Mobile phase:hexane/ethanol (99:1) Flow rate:1.0mL/min Detector:UV254nm Injection:3µL (1mg/mL)</p> 	
<p>OA-2500I    1.06 { -, + } OA-7500    1.13</p>	<p>OA-2500I    1.08 { -, + }</p>	
<p><b>E-03</b>     <b>2,2,2-Trifluoro-1-(9-anthryl)ethanol</b></p>  <p>OA-2000 Column:4.6mmI.D.×25cm Mobile phase:hexane/ethanol (95:5) Flow rate:1.0mL/min Detector:UV254nm Injection:0.5µL (1mg/mL)</p> 	<p><b>E-04</b>     <b>Benzoin</b></p>  <p>OA-4900 Column:4.6mmI.D.×25cm Mobile phase:hexane:ethanol (100:1) Flow rate:1.0mL/min Detector:UV254nm Injection:1µL (1mg/mL)</p> 	
<p>OA-2000    1.40 { -, + } OA-2500I    1.39 { -, + } OA-2500    1.28 { -, + }</p>	<p>OA-3300    1.13 OA-3200    1.11 { +, - } OA-3100    1.07 { +, - }</p>	<p>OA-4900    1.14 OA-2500I    1.10 { S, R } OA-7000    1.07</p> <p>AGP        1.25</p>
<p><b>E-05</b>     <b>α-Cyano-3-phenoxybenzylalcohol</b></p>  <p>OA-4700 Column:4.0mmI.D.×25cm Mobile phase:hexane/1,2-dichloroethane/ ethanol/acetic acid (500:150:5:0.6) Flow rate:1.0mL/min Detector:UV254nm</p> 	<p><b>E-06</b>     <b>Methyl mandelate</b></p>  <p>OA-2000 Column:4.0mmI.D.×25cm Mobile phase: hexane/ethanol (200:1) Flow rate:1.0mL/min Detector:UV230nm</p> 	
<p>OA-4400    1.10 { S, R } OA-4700    1.09 { R, S } OA-4100    1.08 { R, S }</p>	<p>OA-4500    1.05 { R, S }</p>	<p>OA-2500I    1.15 OA-2000    1.06</p>
<p><b>E-07</b>     <b>α-(Trifluoromethyl)benzylalcohol</b></p>  <p>OA-2500I Column:4.6mmI.D.×25cm Mobile phase:hexane/ethanol (99:1) Flow rate:1.0mL/min Detector:UV254nm Injection:5µL (10mg/mL)</p> 	<p><b>E-08</b>     <b>Warfarin</b></p>  <p>OA-2000 Column:4.6mmI.D.×25cm Mobile phase: hexane/ethanol/acetic acid (90:10:0.2) Flow rate:1.0mL/min    Detector:UV254nm Injection:5µL (2.5mg/mL)</p> 	
<p>OA-2500I    1.07</p>	<p>OA-2000    1.22 OA-4900    1.11 OA-4400    1.10</p> <p>AGP        1.42</p>	